

(12) UK Patent Application (19) GB (11) 2 281 966 (13) A

(43) Date of A Publication 22.03.1995

(21) Application No 9318495.0

(22) Date of Filing 07.09.1993

(71) Applicant(s)
Biotrace Limited

(Incorporated in the United Kingdom)

The Science Park, BRIDGEND, Mid Glamorgan,
CF31 3NA, United Kingdom

(72) Inventor(s)
Ian Roy Johnson
Clive Goodfield

(74) Agent and/or Address for Service
Urquhart-Dykes & Lord
Three Trinity Court, 21-27 Newport Road, CARDIFF,
CF2 1AA, United Kingdom

(51) INT CL⁶
G01N 21/01, C12M 1/30 1/34, G01N 21/76


(52) UK CL (Edition N)
G1A AA4 AKA AR7 AT3
G1B BCD

(56) Documents Cited
GB 2207245 A GB 2178847 A EP 0515129 A2
EP 0025350 A2 WO 90/04775 A1

(58) Field of Search
UK CL (Edition M) G1A AKA ARF ARL ARU ARW,
G1B BBC
INT CL⁵ C12M 1/30 1/34, G01N
Online database : WPI

(54) Luminometer

(57) The monitoring instrument comprises a casing 10 having a section 14 which can be pivoted between one position generally flush with a top face of the casing, and a second position which is generally vertical. The pivoted section 14 includes an elongate sample chamber 15 to receive a sample. The instrument has a light detector arrangement for sensing light emitted from a sample inserted into the sample chamber, to provide a measure of the light emitted in a predetermined time period. The instrument is used for monitoring bio-luminescent light emission, in which a swab, pre-moistened with breakage reagent, is wiped over a surface to be tested, then contacted with enzyme solution so that light will be emitted from the swab sample if it has picked up cells: the swab is then inserted into a transparent tube which is placed in the sample chamber 15.

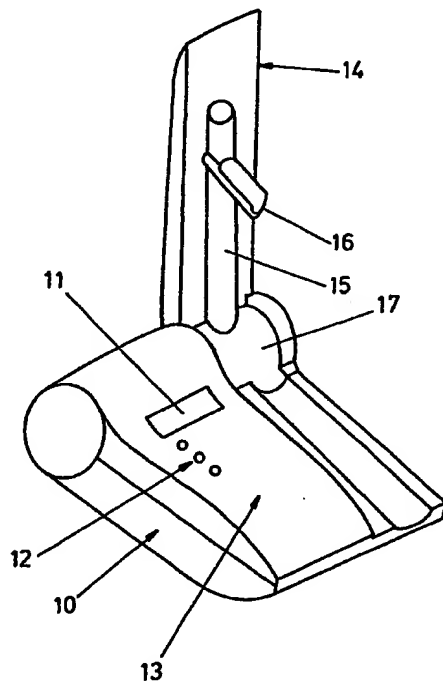

At least one drawing originally filed was informal and the print reproduced here is taken from a later filed formal copy.

The claims were filed later than the filing date within the period prescribed by Rule 25(1) of the Patents Rules 1990.

GB 2 281 966 A

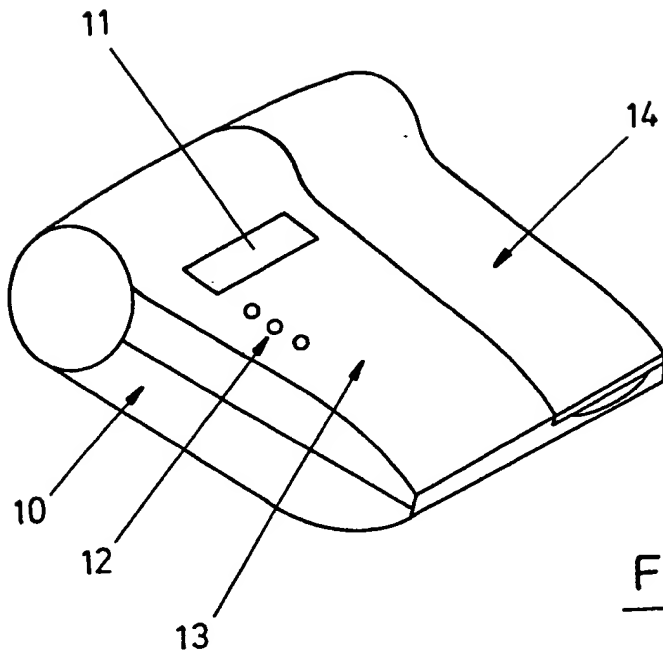


FIG. 1

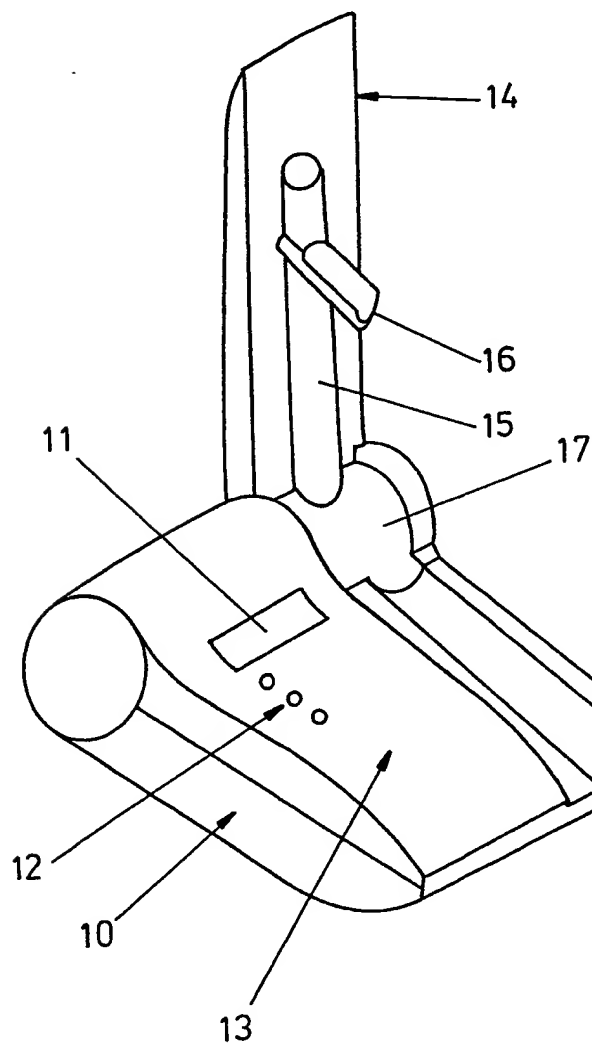


FIG. 2

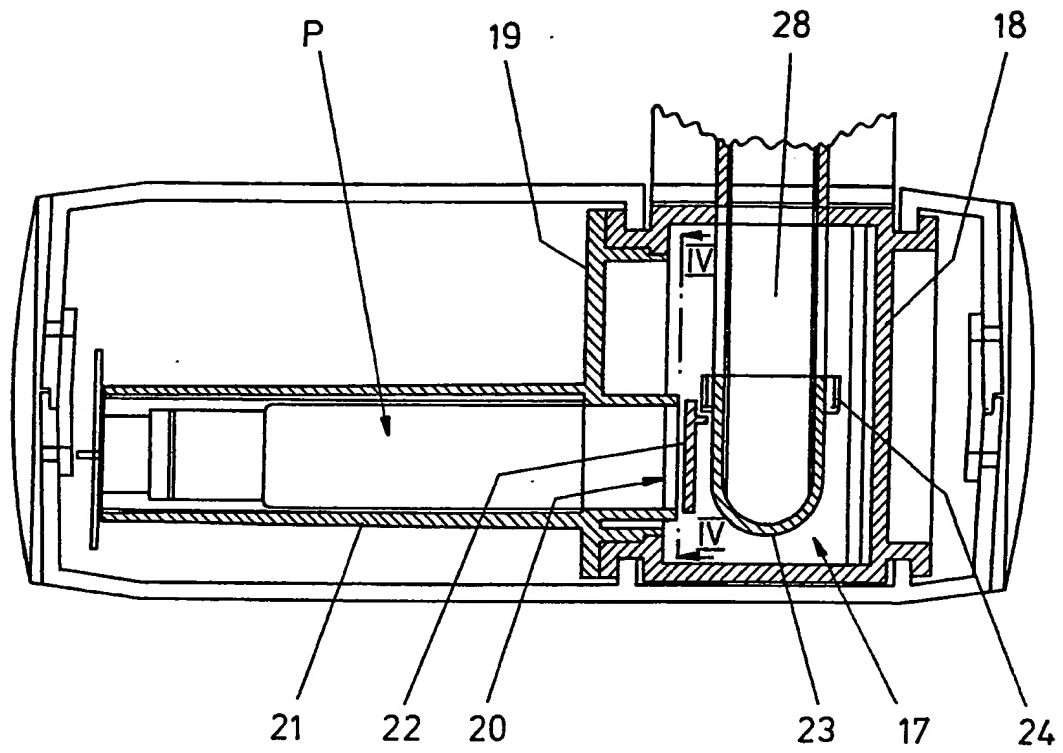


FIG. 3

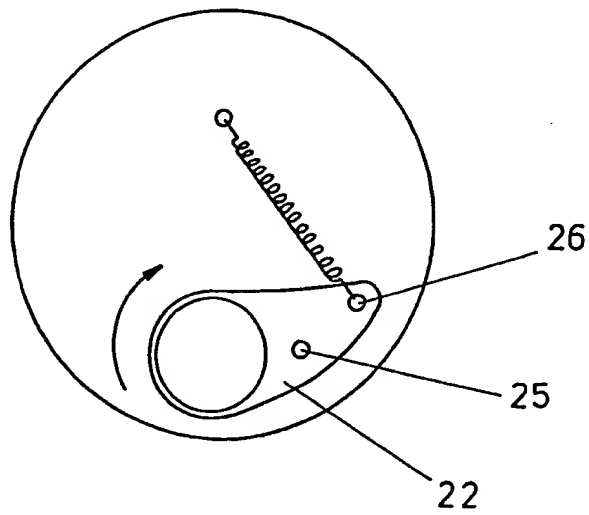


FIG. 4

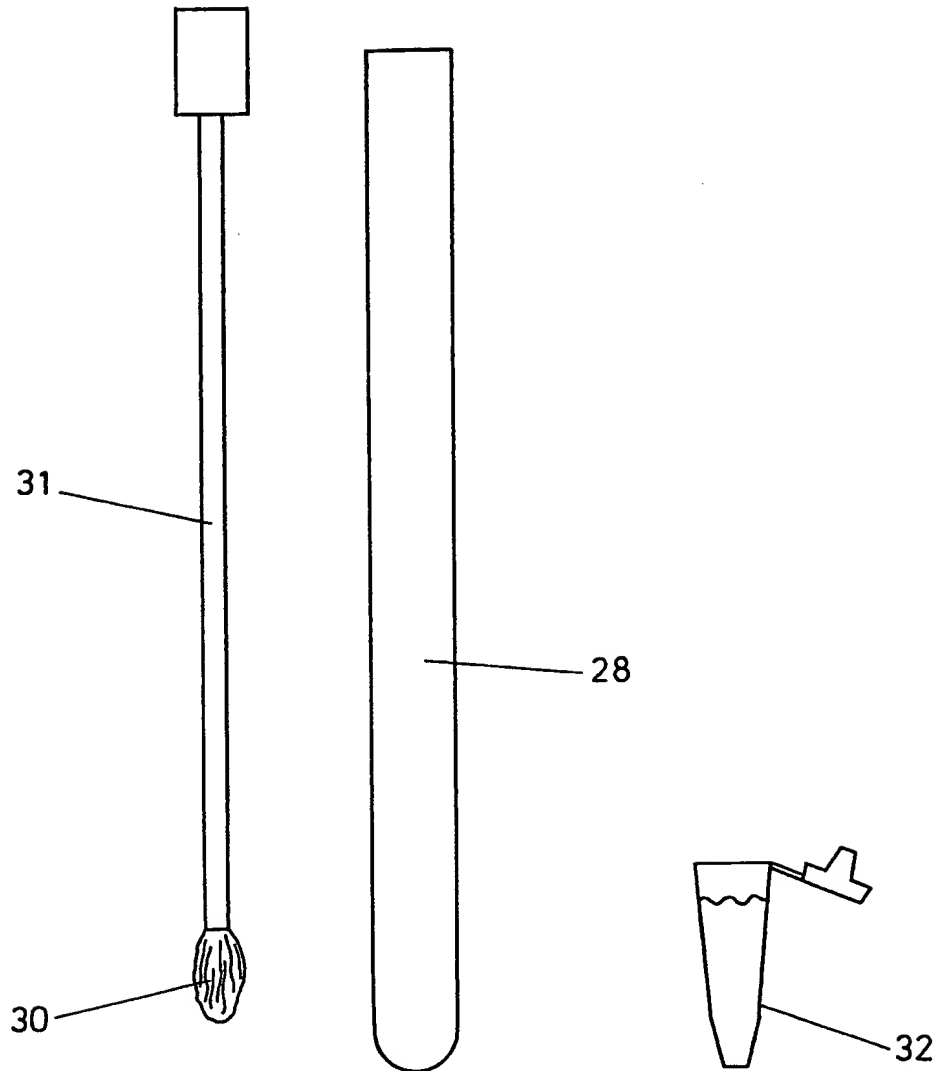


FIG. 5

Bio-luminescence Monitoring Apparatus and Method

This invention relates to an apparatus and method for monitoring bio-luminescent light emission, particularly but not solely for use in hygiene monitoring.

It is known to test for micro-organisms or other cellular material by taking a sample and releasing adenosine triphosphate (ATP) contained within the cells using an appropriate reagent together with the enzyme luciferase in order to cause the emission of light. The light output is related to the concentration of ATP in the sample and hence the contamination present.

Hitherto, a typical testing procedure has involved wiping a pre-moistened swab over a surface to be tested, contacting the swab with a breakage reagent to transfer bacteria or cells from the swab to that reagent and thereby releasing cellular ATP, then transferring the extract to a cuvette containing a liquid of the enzyme luciferase, such that light is now emitted from the liquid in the cuvette. The cuvette is now placed into a light-tight chamber of a monitoring instrument, or luminometer, which measures the light output over a predetermined period of time (typically 10 seconds): this measured light is a measure of the quantity of cells picked up on the swab. The procedure depends upon transferring cells from the surface to the swab and then to the breakage reagent, but in practice this is inefficient because only a proportion of the cells will be transferred.

In accordance with this invention, there is provided a method of testing, comprising wiping a swab, pre-moistened with breakage reagent, over a surface to be tested, contacting said swab with enzyme solution such that if the swab sample has picked up cells, light is now emitted, then measuring the light output directly from the swab.

This method avoids inaccuracies associated with transfer and dilution losses of hitherto known methods using ATP extraction.

The swab is moistened with breakage reagent before it is wiped over the surface to be tested. Preferably a number of swabs are pre-moistened in this manner, then enclosed in

protective tubes until required for use. After wiping over the surface to be tested, preferably the swab is dipped into the enzyme solution for a pre-determined time period (e.g. 60 seconds), then returned to its protective tube. This tube is preferably transparent so that it can then be introduced into the monitor to measure the light now being emitted from the swab owing to the release of ATP from the cells picked up on the swab from the surface being tested. We have found that polyethylene often emits a low level of light, by autofluorescence: we have found that polypropylene does not exhibit autofluorescence and is therefore a suitable material for the protective tubes for the swabs used in this method.

Also in accordance with this invention, there is provided a monitoring instrument (luminometer) comprising a casing having a section which can be pivoted between one position generally flush with a top face of said casing and a second position which is generally vertical, said section including an elongate sample chamber to receive a sample, the instrument further including a light detector arrangement for sensing light emitted from a sample in said chamber and providing a measure of the light emitted in a predetermined time period.

This instrument is able to receive an elongate sample for measurement of its light output: for this purpose the pivoted section is moved to its generally vertical position. However, when not required for use, this pivoted section can be pivoted to its position generally flush with the top face of the instrument casing.

The luminometer is thus able to receive a swab when returned to its protective tube, or sample tube. Preferably a light tight cap is provided for the open top end of the elongate sample chamber, and this cap is slidable into a position in which it detents: in being slid into this position, the cap bears on the top of the sample tube within the sample chamber, to depress the sample tube and correspondingly displace a member on which the sample tube rests; this member now bears against a shutter to pivot the latter from an opening to the light detector.

Embodiments of this invention will now be described by way of example only and with reference to the accompany drawings in which:

FIGURE 1 is a perspective view of a monitoring instrument or luminometer in accordance with this invention, shown with its sample chamber section pivoted to a closed position;

FIGURE 2 is a similar view of the instrument, shown with its sample chamber section pivoted to an in-use position;

FIGURE 3 is an enlarged vertical section across the instrument adjacent its rear edge;

FIGURE 4 is a section on the line IV-IV of Figure 3; and

FIGURE 5 shows a swab, swab protective tube and an enzyme containing tube used with the luminometer in a kit.

Referring to Figures 1 and 2, there is shown a luminometer the housing or casing 10 of which is of generally rectangular, flat form arranged for the monitor to rest flat on a table, bench or the like. The top face of the casing 10 has a window 11 through which a numerical display is presented, a number of translucent windows 12 through which indicator lights (LED's) are visible when energised, and a touch-sensitive panel 13 to operate a "start" switch of the instrument. The luminometer further comprises an elongate section 14 extending from front-to-rear of the casing 10 along its right hand side, this elongate section 14 being pivoted to the casing at the rear of the latter. Normally the section 14 is in a closed position in which it lies flush with the top surface of the casing, as shown in Figure 1, but the section 14 can be pivoted to an upright position as shown in Figure 2.

The pivoted section 14 is formed on its underside with an elongate, tubular chamber 15 which has an open top normally closed by a light-tight cap 16. At its bottom end, the tubular chamber 15 merges into a larger-diameter cylinder 17 which is mounted for pivoting about its axis, to provide the pivotal movement of the section 14. As shown in Figure 3, the opposite ends of cylinder 17 are journaled in fixed annular flanges of the casing 10: one end 18 of the cylinder 17 is closed, whilst

its other end is open but journaled to a fixed circular wall 19 having an integral tube 21 which extends across the width of the casing 10 adjacent its rear edge and bottom wall: the tube 21 houses a photomultiplier P the sensor face of which lies just behind an end 20 of tube 21 which projects into the cylinder 17. A shutter 22 is pivoted to the fixed wall 19 and normally lies across the end 20 of tube 21 to prevent light reaching the photomultiplier P. Alternative forms of light detector may be used instead of the photomultiplier, e.g. an avalanche photodiode or junction light detecting device.

The cylinder 17 has a member 23 slidably mounted in it, as shown in Figure 3. Member 23 is a transparent tube, closed at its lower end, and having a skirt 24 depending from its top and extending around it. The member 23 is biased upwards by a compression spring (not shown). When the member 23 is depressed against the bias of its spring, the lower edge of the skirt 24 bears against a projecting pin 26 on the shutter 22 to pivot the latter about point 25 to its open position (Figure 4).

The luminometer casing 10 houses a pack of rechargeable batteries against its bottom wall and above this a main circuit board is mounted. The liquid crystal display is mounted on a further circuit board above the main circuit board.

In use to measure the light output of a sample, the sample swab is inserted into an elongate plastics sample tube 28 as will be described below. This sample tube 28 is then inserted into the elongate chamber 15 of the section 14, so that its lower end is received by the tubular slidable member 23 in the cylinder 17. Then the cap 16 is pivoted up to an inline position over the top of the elongate chamber 15, and is then pressed down to a position in which it detents: during this movement, the cap 16 bears on the top of the sample tube 28 to press the latter downwards, and in so doing depressing the tubular member 23 against its spring bias, and in turn opening the shutter 22. In its detented position, the cap 16 closes the top of the elongate chamber 15 in light-tight manner, and also operates a switch, preferably a micro-switch to enable the electronic circuit of the monitor.

Now the user starts the luminometer, using the touch-sensitive panel 13, and the light output received by the photomultiplier, in a predetermined period of time, is measured and displayed as a numerical count. The luminometer will not
5 start unless it is enabled by closure of the switch by the cap.

In order to prepare a sample, a swab as shown in Figure 5 is used: the swab 30 is in the form of an absorbent bud on the end of an elongate stalk 31. The swab 30 has been pre-moistened by dipping into an appropriate swabbing solution (ATP
10 breakage reagent), and then stored in an elongate tube. The swab 30 is wiped back-and-forth over e.g. a work-surface to be tested, at the same time turning the stalk 3 so that the whole periphery of the swab 30 will come into contact with the work-surface. During the swabbing, the ATP is released from
15 cellular material picked up from the surface being wiped. The swab is then dipped into a small tube 32 containing enzyme solution so that light is emitted. The swab is then put back into the sample tube 28, which is then introduced into the instrument to measure the light output.

20 Preferably the luminometer is used in a kit which comprises a carrying case for housing the instrument, a plurality of swabs in their protective tubes 28, a plurality of enzyme-containing tubes 32 and a stand for holding the latter tubes. The swab stalk has a plug at its upper end to
25 seal into the top of the tube 28, and the enzyme-containing tube 28 is formed with an integral plug. In use of this kit, the swabs may be pre-moistened and stored in their protective tubes and the tubes filled with enzyme, all at a central laboratory, to enable easy use of the kit in the field, and has
30 the benefit of being "food factory safe" as the kit does not contain any glass or wooden parts which would be hazardous in such environments.

Claims

- 1) A monitoring instrument, comprising a casing having a section which can be pivoted between one position generally flush with a top face of said casing and a second position
5 which is generally vertical, said section including an elongate sample chamber to receive a sample, the instrument further including a light detector arrangement for sensing light emitted from a sample in said chamber and providing a measure of the light emitted in a predetermined time period.
- 10 2) A monitoring instrument as claimed in claim 1, further comprising a light tight closure for the open top end of said elongate sample chamber.
- 3) A monitoring instrument as claimed in claim 2, in which said closure is slidable into a position closing said open top
15 end of the sample chamber, for depressing a sample tube disposed within said chamber, a member being provided on which said sample tube sits, said member being depressed upon depression of said sample tube to cause a shutter of the light detector arrangement to be opened.
- 20 4) A monitoring instrument substantially as herein described with reference to the accompanying drawings.
- 5) A method of testing, comprising wiping a swab, pre-moisted with breakage reagent, over a surface to be tested, contacting said swab with enzyme solution such that if the swab
25 sample has picked up cells, light is now emitted, then measuring the light output directly from the swab.
- 6) A method as claimed in claim 5, in which the pre-moistened swab is enclosed and stored in a protective tube prior to use.
- 30 7) A method as claimed in claim 6, in which the swab is dipped into the enzyme solution for a predetermined time and

then returned to its protective tube.

- 8) A method as claimed in claim 7, in which said protective tube is transparent and is next introduced into a monitor to measure the light emitted from the swab sample.
- 5 9) A method of testing, the method being as claimed in claim 5 and substantially as herein described.

Relevant Technical Fields

- (i) UK Cl (Ed.M) G1A (AKA, ARF, ARL, ARU, ARW)
 (ii) Int Cl (Ed.5) G01N

Search Examiner
 S J MORGAN

Date of completion of Search
 4 AUGUST 1994

Databases (see below)

(i) UK Patent Office collections of GB, EP, WO and US patent specifications.

Documents considered relevant following a search in respect of Claims :-
 1-3

(ii) ONLINE DATABASE:- WPI

Categories of documents

- X:** Document indicating lack of novelty or of inventive step. **P:** Document published on or after the declared priority date but before the filing date of the present application.
- Y:** Document indicating lack of inventive step if combined with one or more other documents of the same category. **E:** Patent document published on or after, but with priority date earlier than, the filing date of the present application.
- A:** Document indicating technological background and/or state of the art. **&:** Member of the same patent family; corresponding document.

Category	Identity of document and relevant passages	Relevant to claim(s)
X	GB 2207245A (UNILEVER) see whole document	1
X	EP 0515129 A2 (ISRAEL AIRCRAFT) see whole document	1
X	EP 0025350 A2 (DYNATECH) see whole document	1

Databases: The UK Patent Office database comprises classified collections of GB, EP, WO and US patent specifications as outlined periodically in the Official Journal (Patents). The on-line databases considered for search are also listed periodically in the Official Journal (Patents).

Patents Act 1977 Examiner's report to the Comptroller under Section 17 (The Search report)	Application number GB 9318495.0
Relevant Technical Fields (i) UK Cl (Ed.M) G1A (AKA) G1B (BBC) (ii) Int Cl (Ed.5) C12M G01N Databases (see below) (i) UK Patent Office collections of GB, EP, WO and US patent specifications. (ii) ONLINE DATABASE: WPI	Search Examiner S J MORGAN
	Date of completion of Search 1 DECEMBER 1994
	Documents considered relevant following a search in respect of Claims :- 5-9

Categories of documents

X: Document indicating lack of novelty or of inventive step.	P: Document published on or after the declared priority date but before the filing date of the present application.
Y: Document indicating lack of inventive step if combined with one or more other documents of the same category.	E: Patent document published on or after, but with priority date earlier than, the filing date of the present application.
A: Document indicating technological background and/or state of the art.	&: Member of the same patent family; corresponding document.

Category	Identity of document and relevant passages	Relevant to claim(s)
A	GB 2178847 A (PHILIPS)	
A	WO 90/04775 A1 (BIOTRACE)	

Databases: The UK Patent Office database comprises classified collections of GB, EP, WO and US patent specifications as outlined periodically in the Official Journal (Patents). The on-line databases considered for search are also listed periodically in the Official Journal (Patents).